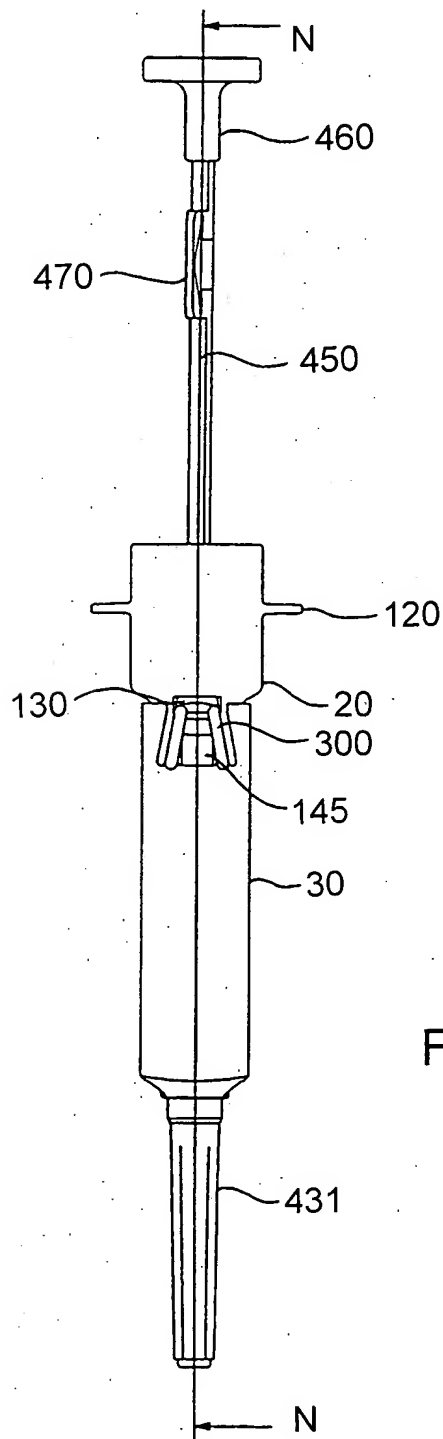



FIG. 1

## Page 2 of 25



FIG. 2



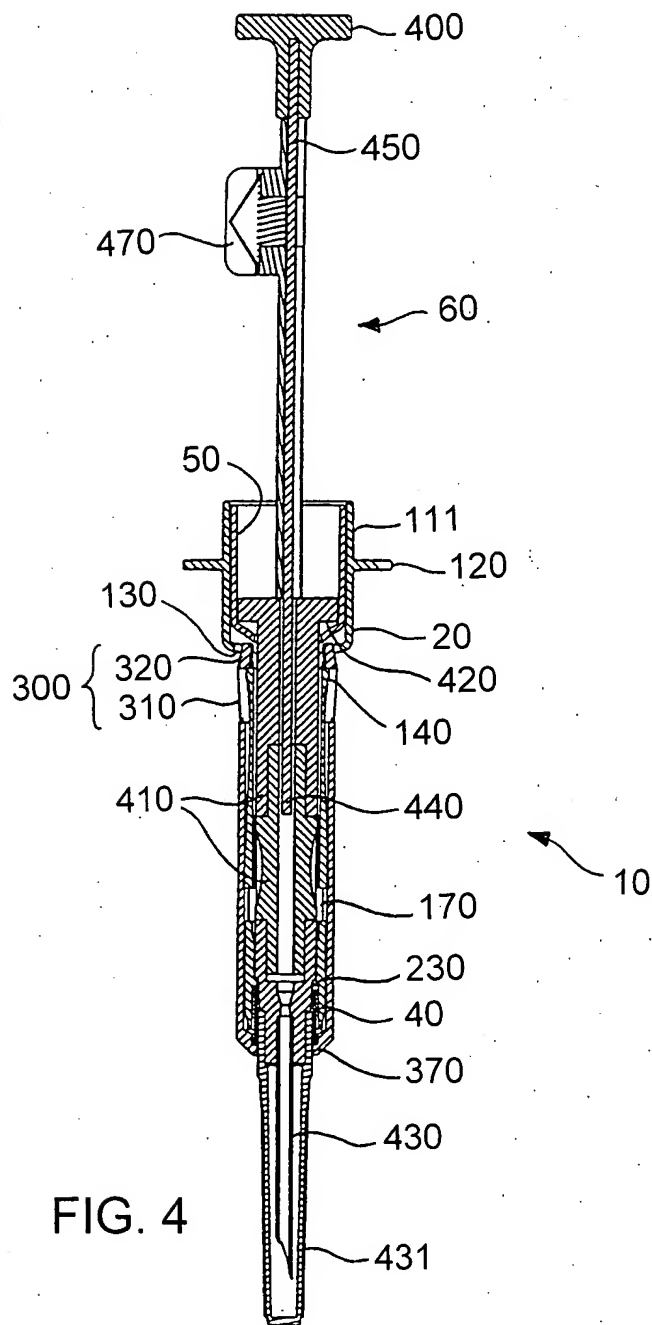

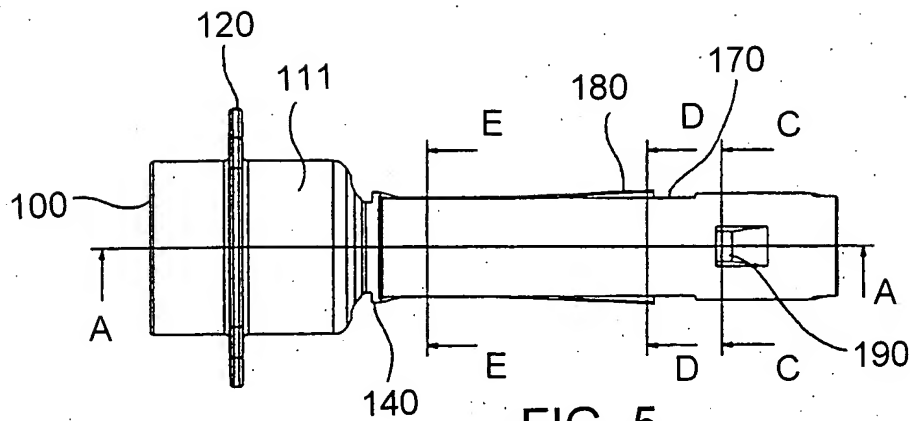


FIG. 5




FIG. 6




FIG. 7




FIG. 8

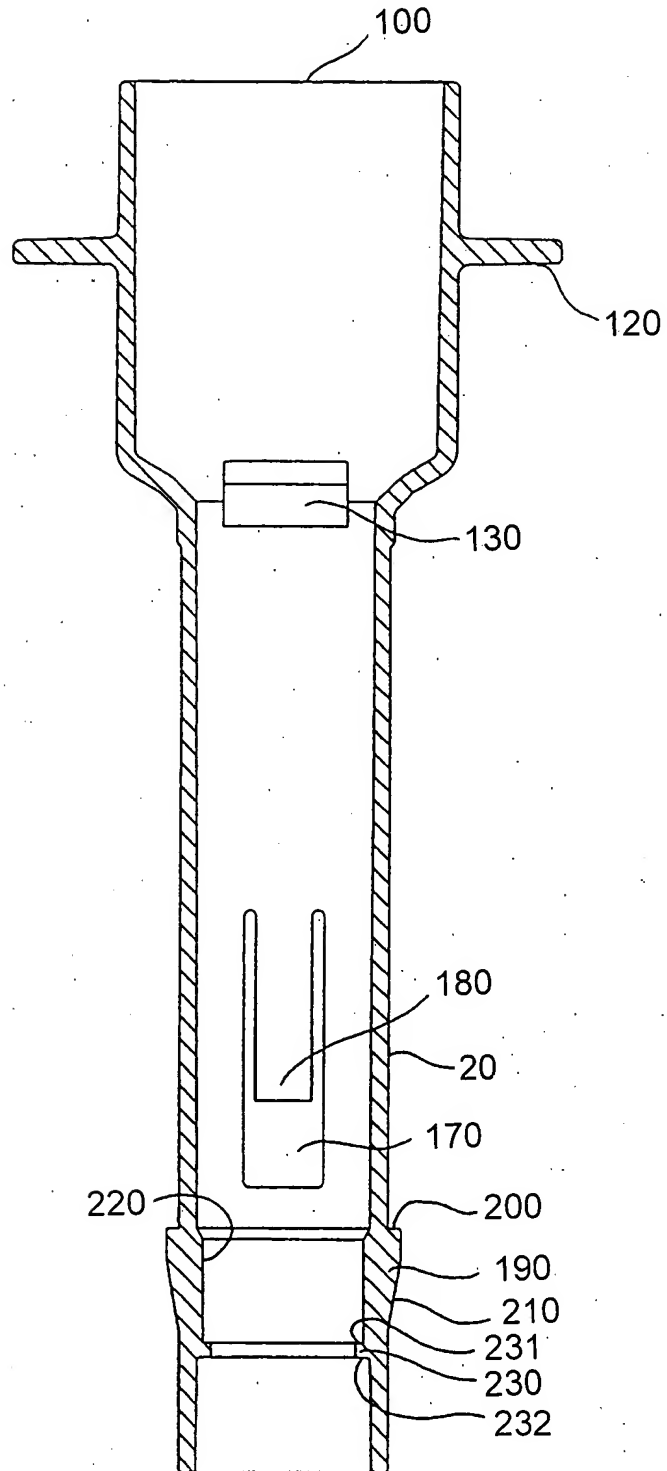


FIG. 9

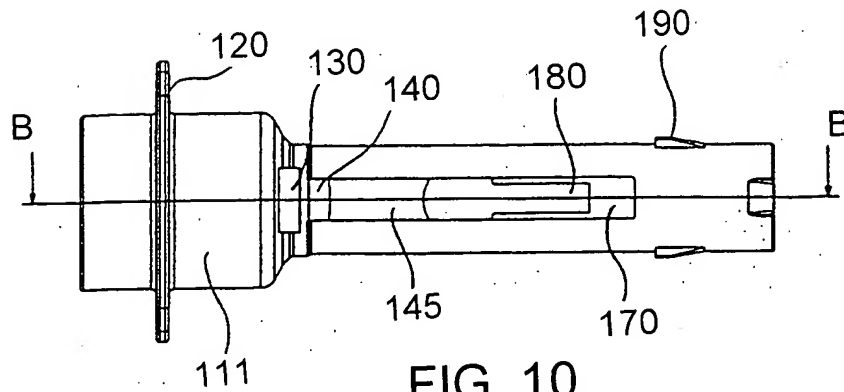


FIG. 10

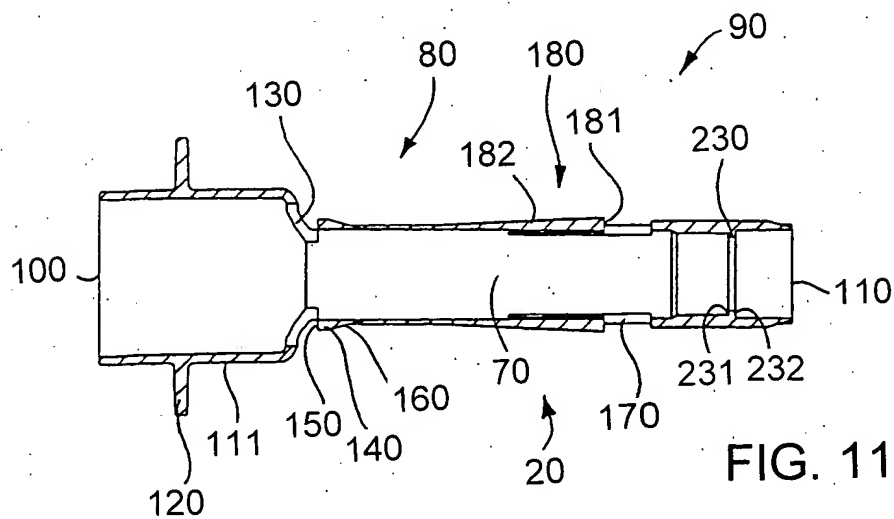


FIG. 11

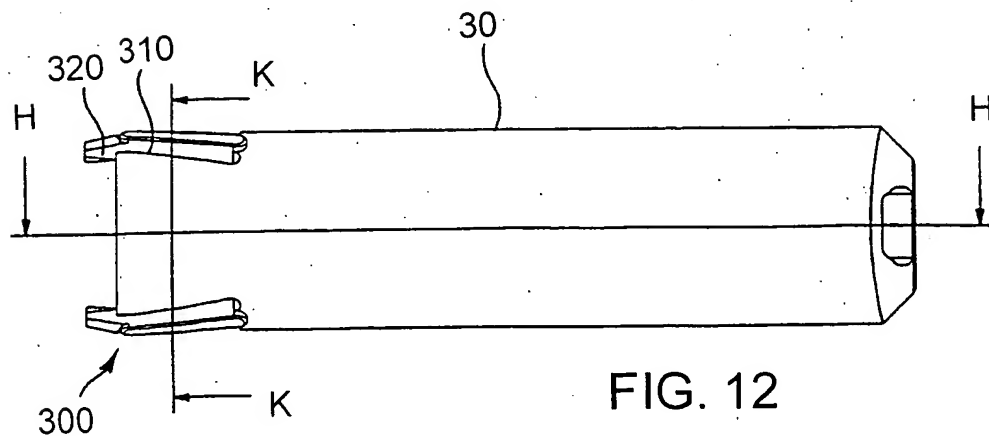
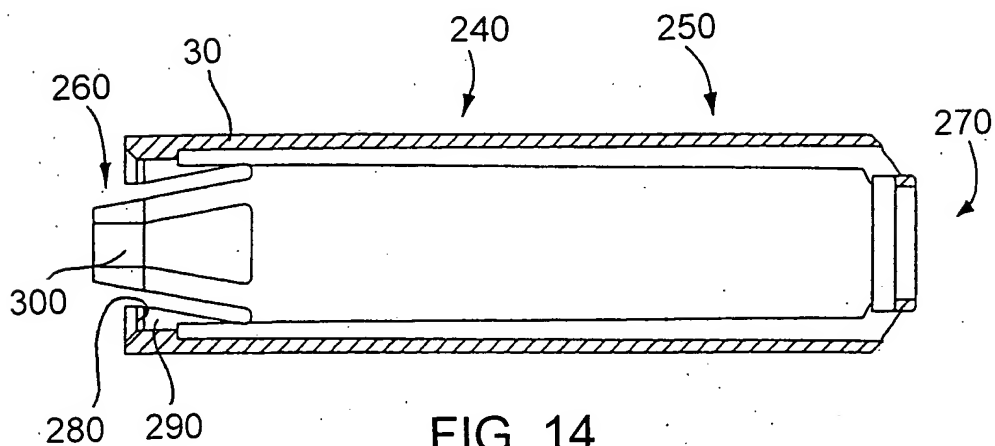
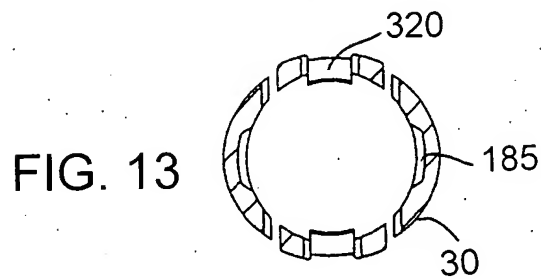


FIG. 12





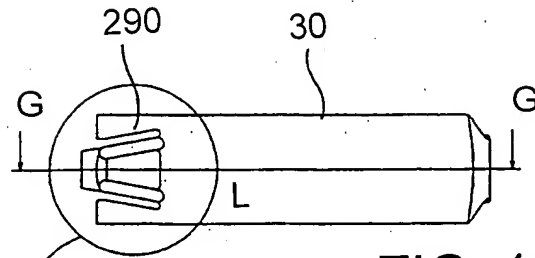


FIG. 15

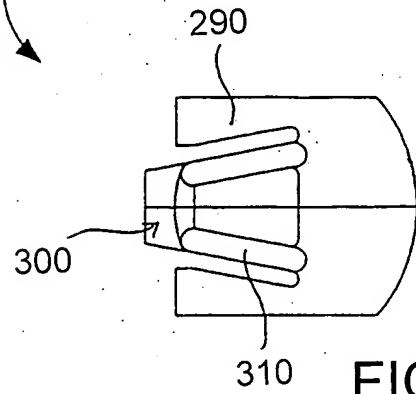


FIG. 15A

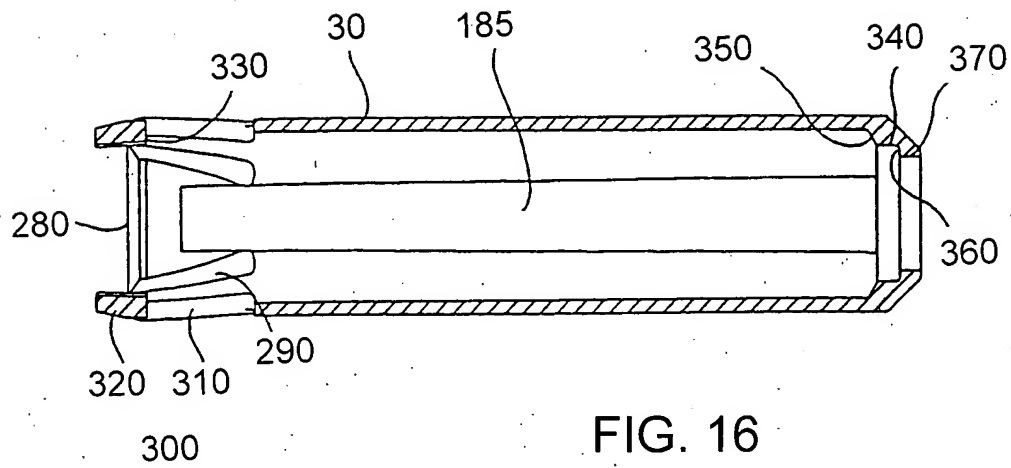
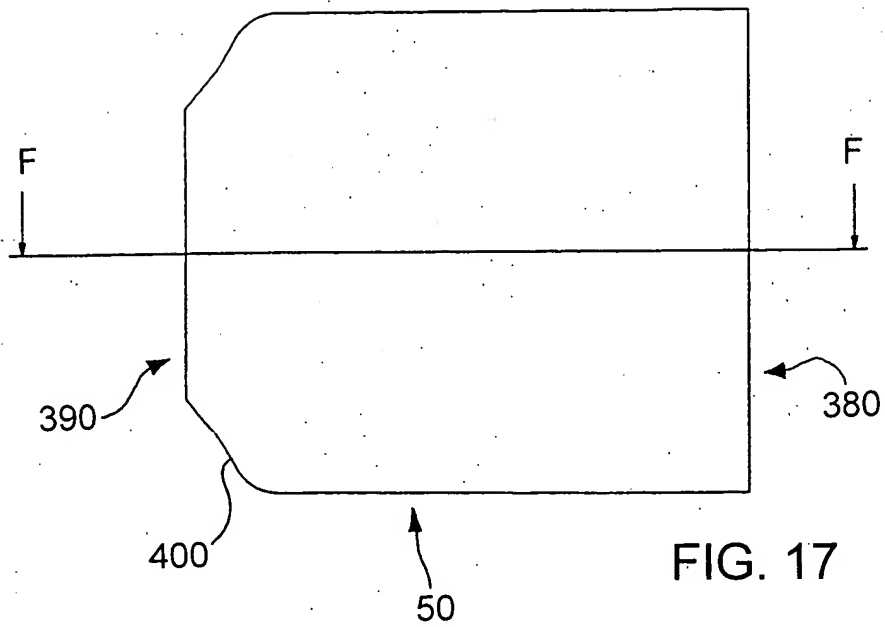
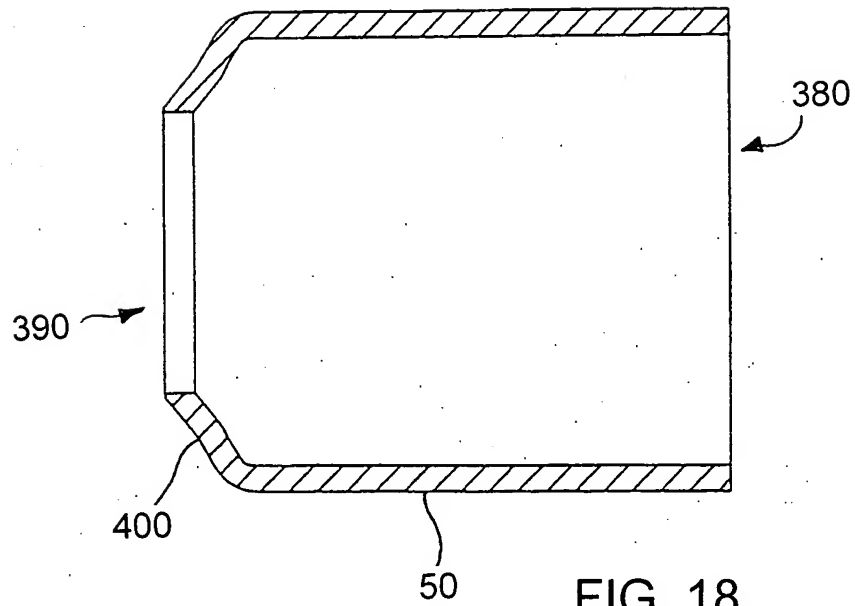


FIG. 16





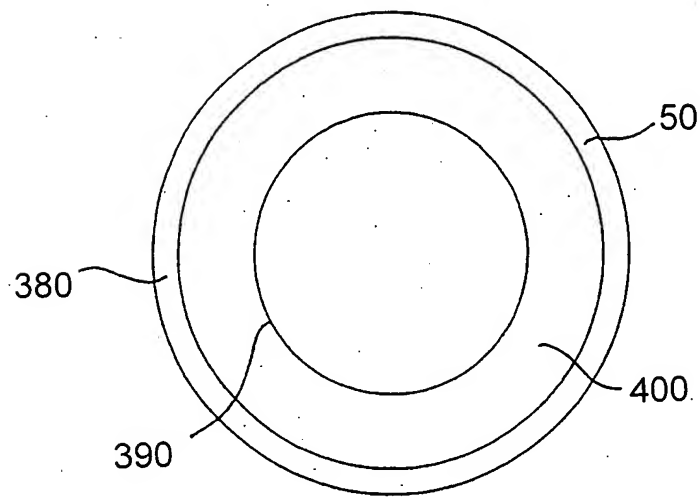
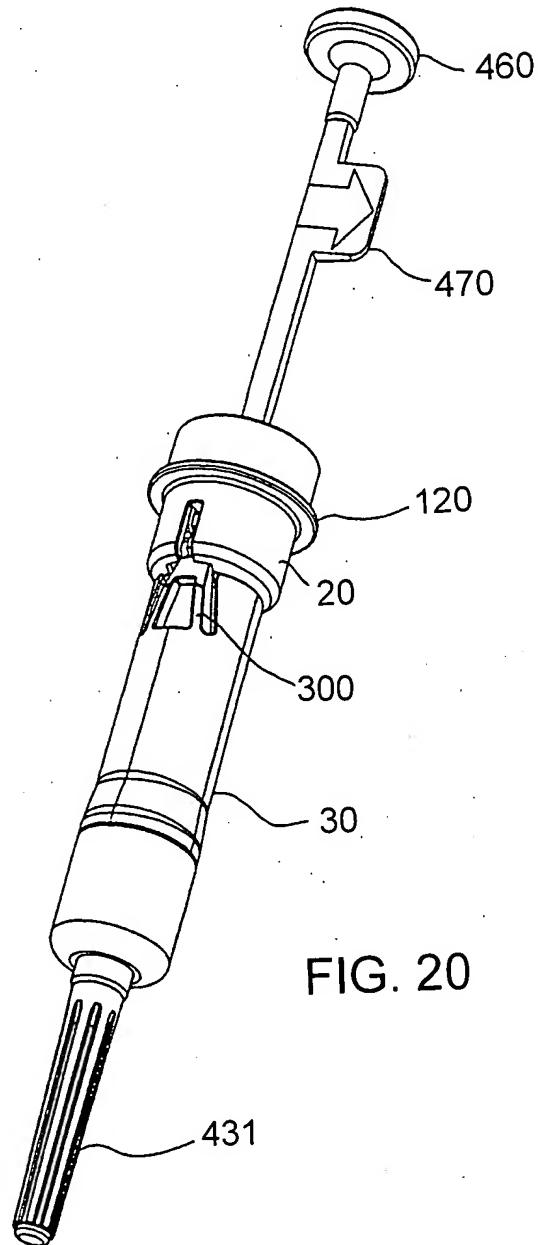
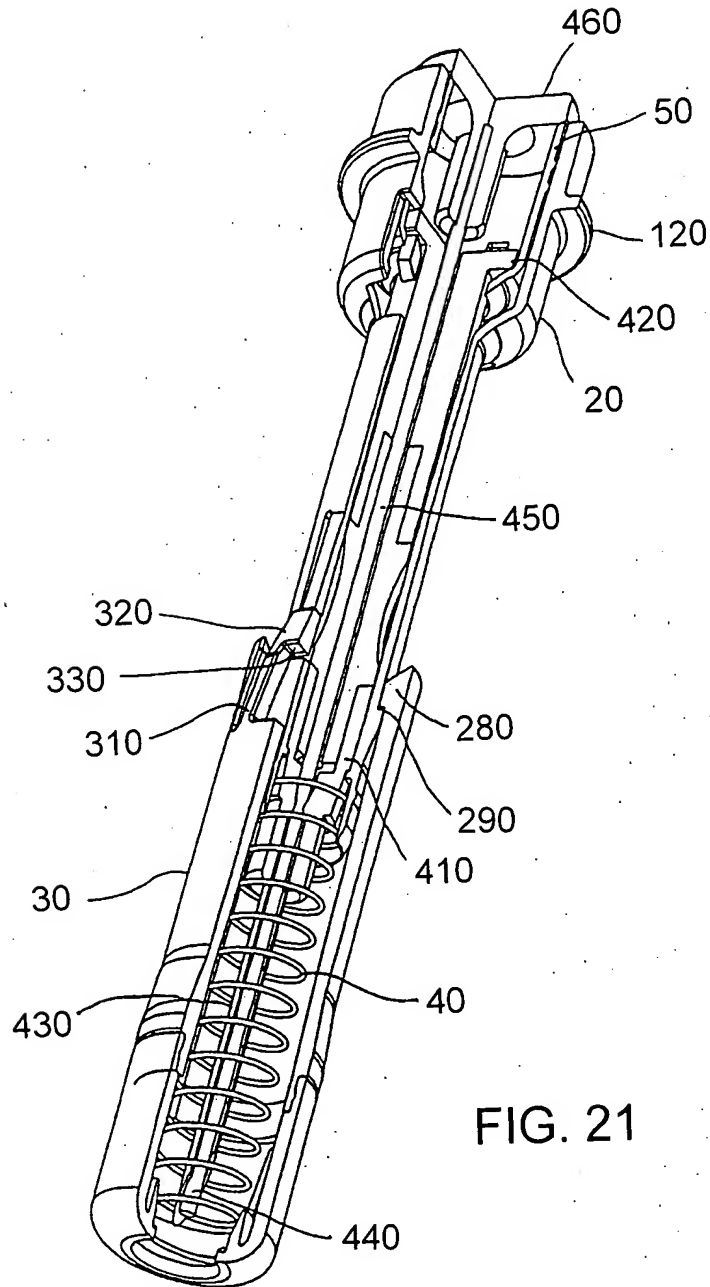


FIG. 19

AUTOMATICALLY OPERABLE SAFETY SHIELD SYSTEM  
FOR SYRINGES





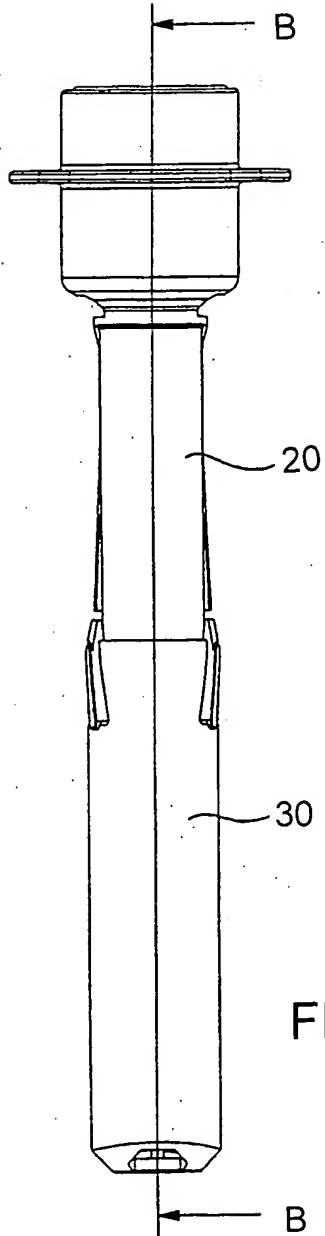


FIG. 22



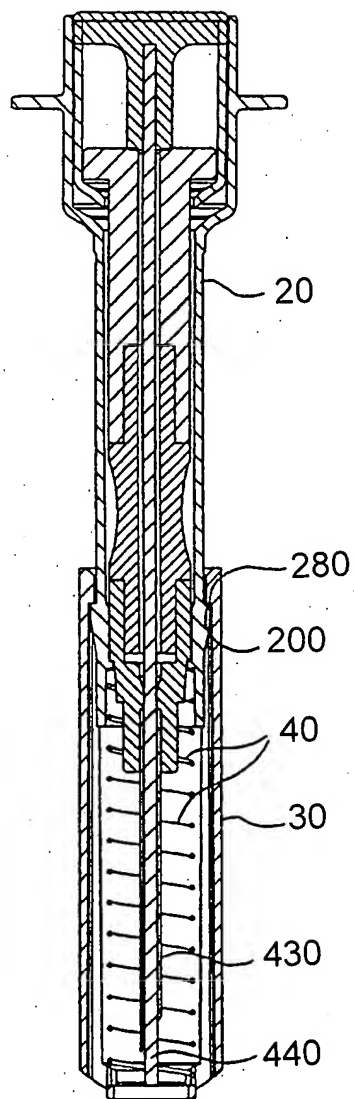


FIG. 23

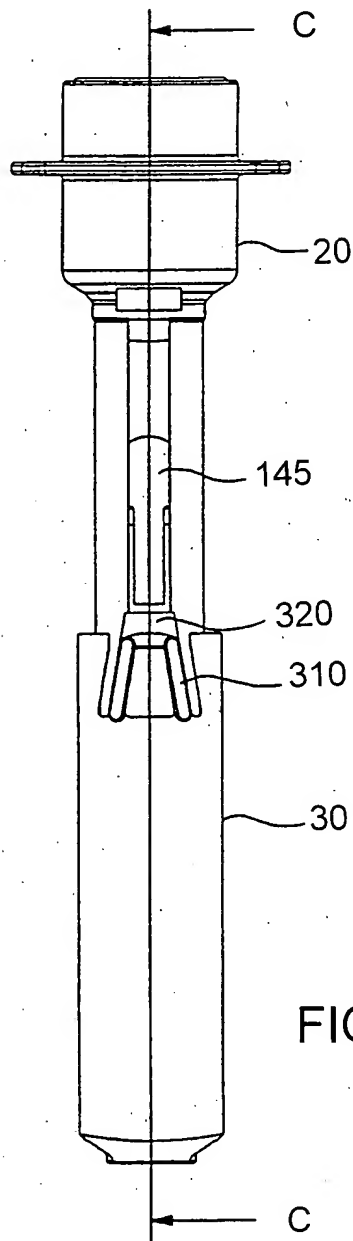
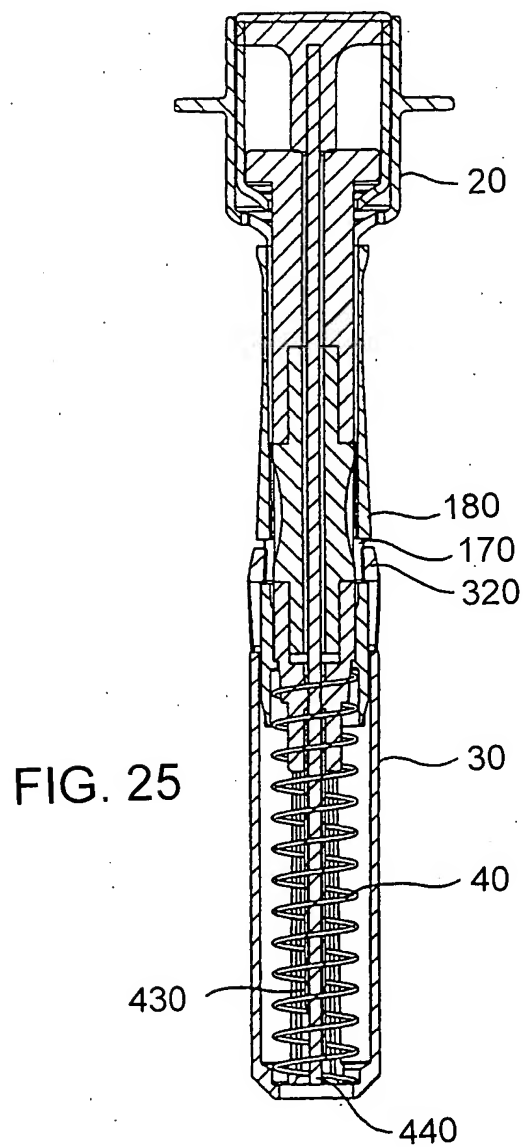
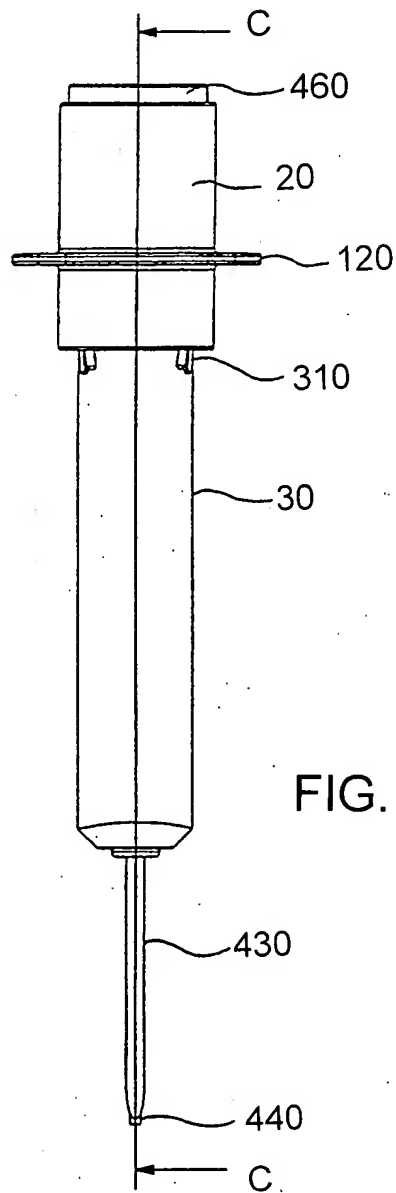


FIG. 24





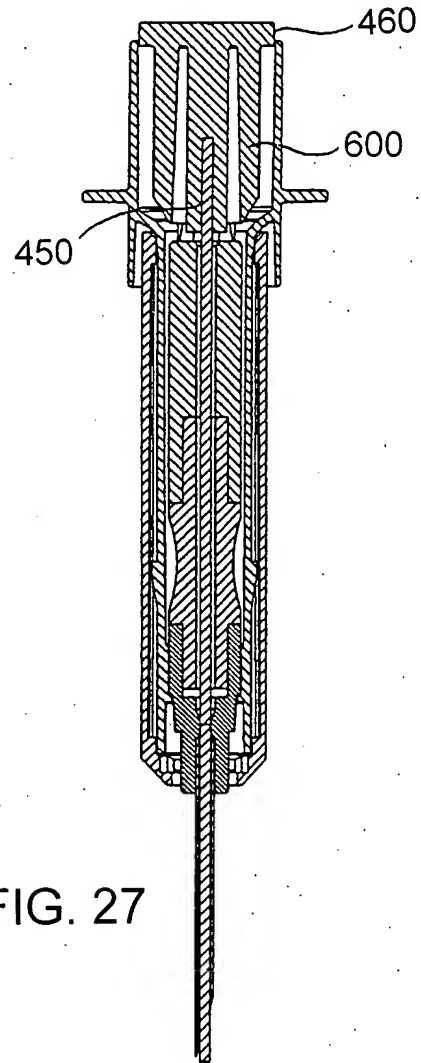
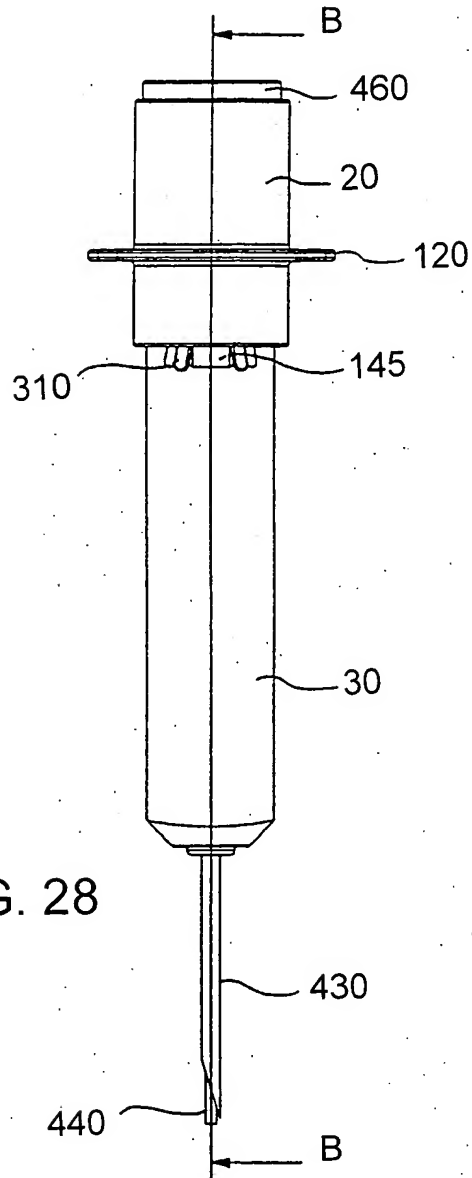


FIG. 27



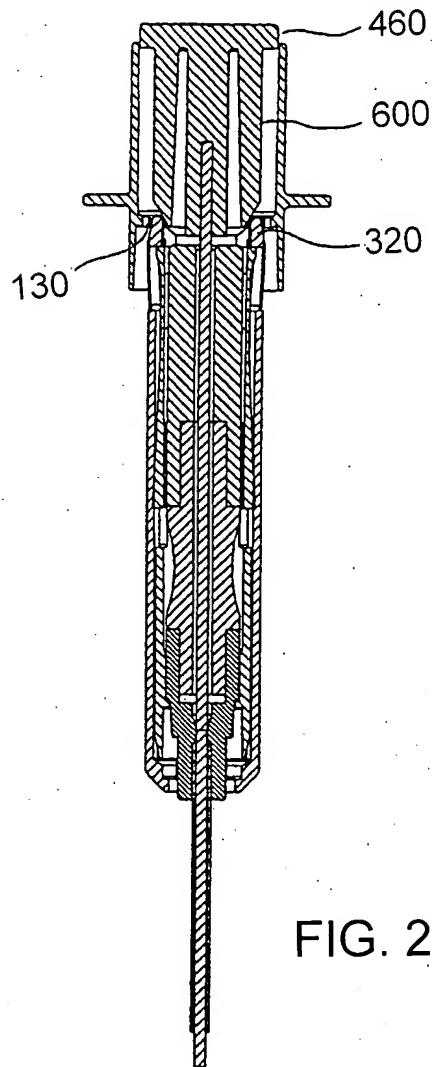


FIG. 29

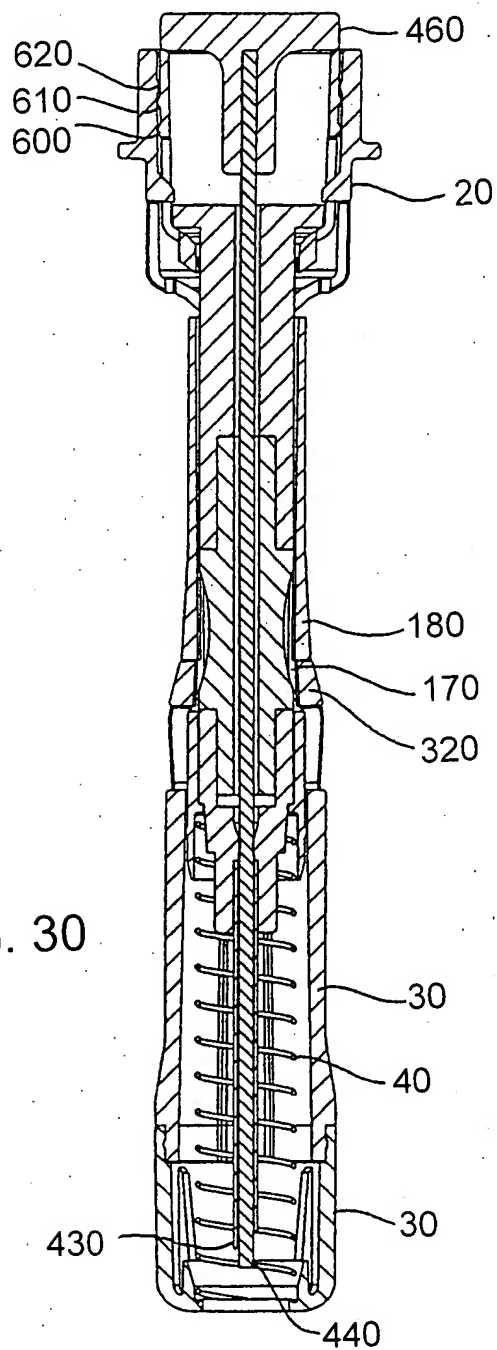


FIG. 30



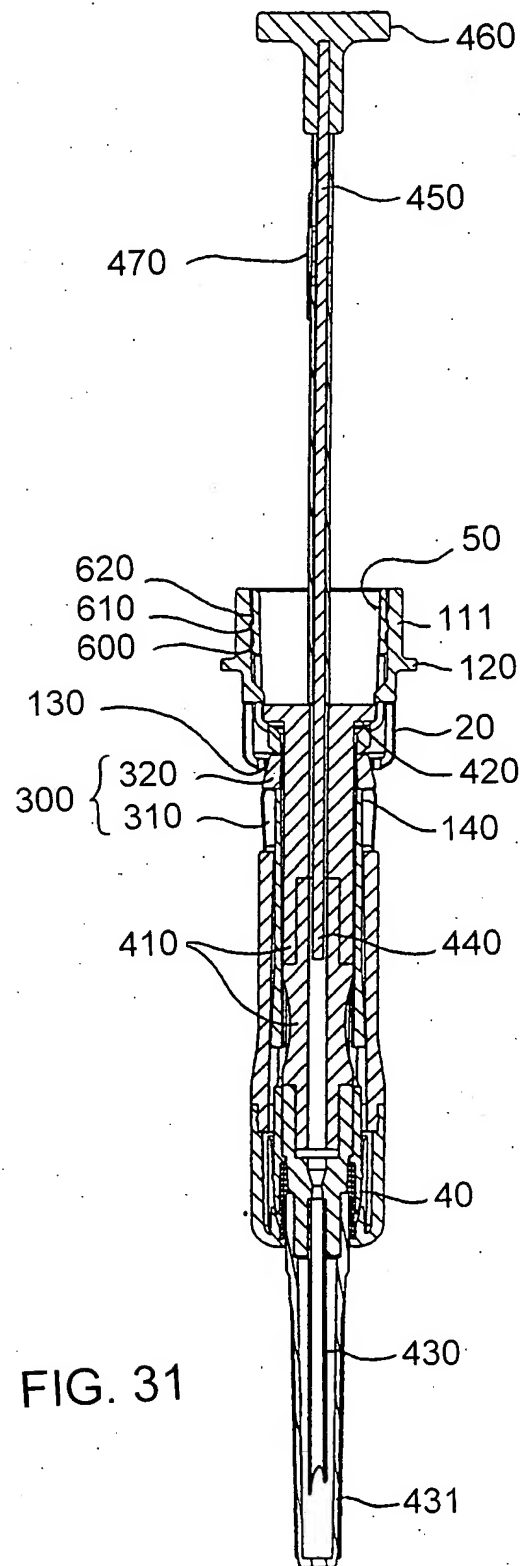


FIG. 31